

POWERFUL CARDIAC MONITORING



Reveal LINQ™
Insertable Cardiac Monitoring System

Patient Registration Guide

QUICK STEPS

1. Visit myorders.medtronic.com.
2. Enter LOGIN and PASSWORD to access the Registration Portal.
3. LOGIN: Email: _____ Password: _____
4. Click **Register a New Device**.
5. Fill out each tab, clicking Continue to Next Step after each step is complete. Required information has a red asterisk, and you will not be able to proceed until all required information is completed.
 - a) Tab 1: **Patient and Hospital**
 - Enter patient information, providing all available details
 - Select procedure facility from the drop-down list
 - b) **New!** Select "Enroll in CareLink" to automatically notify the patient's follow-up clinic to add a new patient.
 - c) Tab 2: **Physician Details**
 - **Procedure Physician tab** – Select a doctor from the **Choose a Physician** drop-down list or select **Add New Physician** entry and provide the available details for this physician
 - **Follow-Up Physician, Follow-Up Clinic and Referring Physician** – Enter information using the respective tabs
 - d) Tab 3: **Procedure and Remote Follow-Up Details**
 - Enter the Reason for Monitoring
 - Enter the venue where the procedure occurred
 - Enter the device details – The serial number can be found on the device box or stickers from the device box. The serial number is formatted as YDM#####A. Enter the **Monitor Delivery Method** and **Serial Number** for the MyCareLink Patient Monitor.
 - Skip REPLACED device portion
 - e) Tab 4: **Review**
 - Review the full registration and select Submit to send this information to Medtronic's device tracking registry
6. Save or Email Registration.
 - a) After submitting, you may save a hard copy of this registration by selecting the **Save as PDF** option on the upper right of the summary.
 - b) If you wish to send the patient registration information to a physician's clinic, **enter the recipient's email address** and select **Send Email**. Repeat with any additional individuals who wish to receive this information. **Note:** This is not required if you selected to enroll the patient in CareLink.
 - c) To email to Dr. _____ office: (add email address) _____
7. To LOG OUT
 - a) Click **Welcome, LINQ User** on the top right
 - b) Select **Log Out**

TIPS FOR NAVIGATION

Thank you for selecting Reveal LINQ Insertable Cardiac Monitoring. The intent of this Patient Registration Guide is to help you get started registering Reveal LINQ patients on the Medtronic myOrders website. The guide consists of two sections:

- Setting up a User Account
- Registering a Patient

For optimal navigation within the registration website, use the tabs and “Continue to Next Step” or “Previous Step” buttons within the registration screens. Avoid using the back/forward arrows on your Internet Browser.

New Registration

1. Patient & Hospital | 2. Physician Details | 3. Implant & Other Details | 4. Review Registration Details

Step 1: Patient Details Required *

Basic Patient Details	Patient Address	Procedure Hospital
First Name* <input type="text"/>	Address Line 1* <input type="text"/>	Name of Hospital* Please Select ▼
Middle Name <input type="text"/>	Address Line 2 <input type="text"/>	Account # <input type="text"/>
Last Name* <input type="text"/>	City* <input type="text"/>	City <input type="text"/>
Gender <input type="radio"/> Female <input type="radio"/> Male	State* Please Select ▼	State <input type="text"/>
Phone Number* <input type="text"/>	Zip Code* <input type="text"/>	CareLink Enrollment If you do not enroll this patient in CareLink, you will not be able to follow this patient remotely. <input checked="" type="radio"/> Enroll in CareLink <input type="radio"/> Do not enroll in CareLink
Date of Birth* Month ▼ Day ▼ Year ▼	Country* United States of America ▼	
Social Security Number <input type="text"/>		

Continue to next step ▶

Troubleshooting/Help

For assistance with the myOrders website, please contact Customer Service at 1 (877) 527-3426.

SETTING UP A USER ACCOUNT

1. Log onto Medtronic myOrders at myorders.medtronic.com.
2. Select **Request Access**.



3. Fill out all fields and in the Questions/Comments box, type **“Request for device registration.”**
4. Review all information and select **“Submit.”** You will receive confirmation of your User Account within 2 days.

Request Access to My Orders

Please complete the form below to begin the process of setting up your My Orders account.

Your Information Required *

Name*:

Title*:

Email Address*:

Phone Number*: Ext*:

Fax:

Account Number:

Facility Name*:

Street Address*:

City*:

State/Region*:

Zip/Postal Code*:

Country:

Don't know your account number?
Please contact your purchasing department as providing your account number will expedite your account set-up.


Questions/Comments

REGISTERING A PATIENT

1. Access Medtronic myOrders at myorders.medtronic.com, enter your email and password, and select **Log In**.




2. Click **Register a New Device**. Note: Previous Registrations are listed on your home page, "My Dashboard." Customers will be able to see the registration history for their entire facility, providing a more comprehensive view of the account's registration history. Access to each facility's registrations is based on account selection in the user's profile.

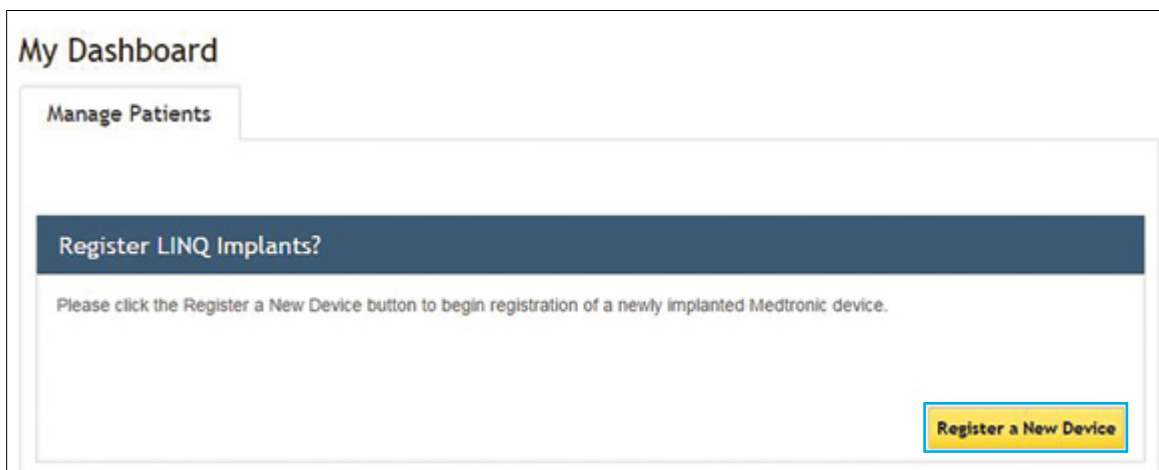

REGISTERING A PATIENT *(continued)*

3. Select Registration Type:

- a) Cardiac Monitor
- b) Select **Continue Registration**.

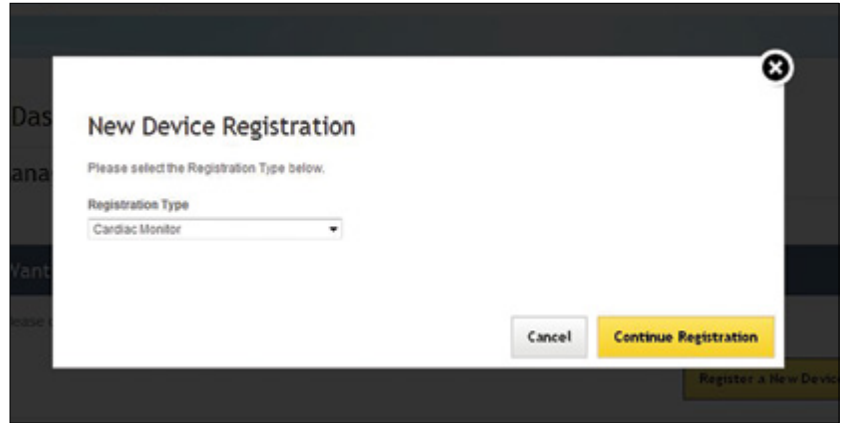

4. Tab 1: Patient and Hospital

- a) Enter patient information on the Patient & Hospital tab, providing all available details; this will ensure accurate records for device tracking and prompt delivery of the patient ID card.
- b) **New!** Select "Enroll in CareLink" to automatically notify the patient's follow-up clinic to add a new patient.
- c) When complete, select **Continue to Next Step**.

REGISTERING A PATIENT *(continued)*

5. Tab 2: Physician Details

- a) Within the Procedure Physician tab, select a doctor from the **Choose a Physician** drop-down list. The details for this physician will automatically display.
- b) If the correct doctor is not yet listed, please select the **Add New Physician** entry and provide the available details for this physician. This physician will then be available to select for future registrations.
- c) Enter Follow-Up Physician and Referring Physician information using the respective tabs. To search for a physician, search by last name and state.
- d) Enter Follow-Up Clinic information under the Follow-Up Physician tab. If the correct clinic is not listed, select Search for a Clinic to locate.
- e) When complete, select **Continue to Next Step**.

New Registration

1. Patient & Hospital | **2. Physician Details** | 3. Implant & Other Details | 4. Review Registration Details

Associated Physician's Information Required *

Procedure Physician | Follow-Up Physician | Referring Physician

Choose Another Physician: Douglas Hodgkin Or Search a Physician

Physician Record #
1338019229421000

First Name*
Douglas

Middle Name
David

Last Name*
Hodgkin

Phone*
763-425-2000

Email Address
dhodgkin@northwestern

Address Line 1*
3300 Oakdale Ave N, Ste 200

Address Line 2

City*
Minneapolis

State*
Minnesota

Zip Code*
55412-0805

Country*
United States of America

CareLink Clinic Information

Name of Clinic* Or Search for Clinic*

Clinic Name*

State*
Please Select

CareLink Clinic Information

▲ Please complete your clinic search
▲ Please provide the Clinic Name and State.

Name of Clinic*

State*
Please Select

Or Search for Clinic*

REGISTERING

A PATIENT *(continued)*

6. Tab 3: Procedure & Remote Follow-Up Details

- a) Within the Procedure & Remote Follow-Up Details tab, select:
 - i. The **Reason for Device** which has prompted the patient to receive a Reveal LINQ ICM
 - ii. The **Procedure Venue** where the procedure occurred
 - iii. The **Procedure Date** and **Serial Number** for the Reveal LINQ ICM
 - iv. The **Monitor Delivery Method** and **Serial Number** for the MyCareLink Patient Monitor
- b) **Optional:** If the patient had an existing product which is being replaced by the Reveal LINQ ICM, check the box labeled Replaced (Yes/No) and provide the details on the previously implanted device.
- c) **Optional:** If the Reason for Device requires more details, select "other" under Reason for Device and use the Reason for Device details box to communicate to the clinic.
- d) Use the Notes box to include additional information to be processed with this registration.
- e) When complete, select **Continue to Next Step**.

Step 3: Procedure & Remote Follow-Up Details

Submitter's Details

First Name : Last Name : Notes :

Email Id : Phone :

Procedure Details

Reason for Monitoring* Reason For Monitoring Detail Procedure Venue*

Implant Date *	Mfg *	Device Model Number *	Device Serial Number *	Side of Body(R/L) Heart Chamber	Device Type *
Mont <input type="text" value="▼"/> Day <input type="text" value="▼"/> Year <input type="text" value="▼"/>	<input type="text" value="MDT"/>	<input type="text" value="LNQ11"/>	<input type="text" value=""/>	<input type="text" value="Select"/>	<input type="text" value="Reveal LINQ"/>
Device Implanted Today?					
Replaced (Yes/No)	Replaced Mfg.*	Replaced Device Model Number *	Replaced Device Serial Number *	Replaced Device Status *	
<input type="checkbox"/> Yes	<input type="text" value="MDT"/>	<input type="text" value="Select"/>	<input type="text" value=""/>	<input type="text" value="Select"/>	

Monitor Details

Please select CareLink Monitor Details below. Entering the monitor serial number does not imply the patient is enrolled in Carelink. Follow up requires the patient to be enrolled in Carelink.

Monitor Delivery Method* Monitor Model Number Monitor Serial Number

REGISTERING A PATIENT *(continued)*

7. Tab 4: Review

- a) Within the Review screen, review the full registration, edit if needed, and select **Submit** to send this information to Medtronic's device tracking registry.

Step 4 : Review

Basic Patient Details > Edit

Name: Jane Doe
Gender: -
Phone Number: 632-134-4322
Social Security Number: -
Date of Birth: 07/03/1977
CareLink Enrollment: Yes
Address: 123 Oaklane Ct, Blaine, Minnesota, 55419, United States of America

Implant Hospital Details > Edit

Name of Hospital: North Memorial Heart and Vascular Institute
Address: Minneapolis, Minnesota
Account #: 0001141736
Calibration Constant: N/A
Procedure Venue: Hospital Outpatient

Physician Info > Edit

Procedure Physician

Physician Record #: 100015330211027
Name: Scott Hoppe
Address: 3300 Oakdale Ave N, Ste 200, Robbinsdale, Minnesota, 55422-2926, United States of America
Email: shoppe2332@yahoo.com
Phone Number: 763-225-2222

Follow-Up Physician

Physician Record #: 10001522421002
Name: Douglas David Hodgson
Address: 3300 Oakdale Ave N, Ste 200, Minneapolis, Minnesota, 55422-2926, United States of America
Email: ddg.hodgson@northmemorial.com
Phone Number: 763-225-2222
[CareLink Clinic](#)
Hospital Name: Fairview Riverside Hospital
Account #: 0001129192

Referring Physician

Physician Record #: 10001522421002
Name: Douglas David Hodgson
Address: 3300 Oakdale Ave N, Ste 200, Minneapolis, Minnesota, 55422-2926, United States of America
Email: ddg.hodgson@northmemorial.com
Phone Number: 763-225-2222

Registration Type: Cardiac Monitor

Reason for Device: Cryptogenic Stroke

Reason For Device Detail: -

Procedure Details > Edit

Implant Date	MTG	Device Model Number	Device Serial Number	Side of Body (R/L) Heart Chamber	Device Type
09/1/2015	MDT	LVQ11	RLA1220750	-	Reveal LQD
Replaced (Yes/No)	Replaced MTG	Replaced Device Model Number	Replaced Device Serial Number	Replaced Device Status	
No	-	-	-	-	

Monitor Details

If you selected "Do Not Subscribe" this patient will not be enrolled in CareLink.

Monitor Delivery Method: Distribute at Clinic

Monitor Model Number: -

Monitor Serial Number: -

Submitter Details

Submitted By: Mark Lutzer
Email: mark.lutzer@gmail.com
Phone: 123-233-3334

Notes

← Previous Step
Submit >

All patient and clinic data are fictitious and for demonstration purposes only.

EMAIL REGISTRATION

b) After submitting, can email a copy of this registration to the follow-up physician's clinic, entering the recipient's **email address** and select **Send Email**. **Note:** If you chose to enroll the patient in CareLink, you do not need to send an email. An email is required only for patients not enrolled.

c) Manage Contacts

- Click on "Add/Edit Contacts" to save and update email addresses that will be used frequently
- Click on "Add Row" to add multiple contacts at one time

Registration Successfully Completed!

The registration has been successfully submitted to Medtronic. The patient's follow-up clinic has been successfully notified of their new patient in CareLink.

If you would like to email a copy of the registration, use the box below.

Enter Email/Name/Clinic **Send Email** | Add/Edit Contacts **Save/Print as PDF**

Tip: Click on 'Add/Edit Contacts' to save and update email addresses that will be used frequently.

Tip: You can add multiple email addresses using a semicolon ";" between each recipient.

Home > New Registration

Add/Edit Contacts

Add a New Contact | **Edit a Contact**

First Name	Last Name	Email*	Associated Clinic
<input type="text"/>	<input type="text"/>	<input type="text"/>	<input type="text"/>

Add Row **Cancel** **Save**

Delete Selected Record(s)

d) If you would like to email a group of people regularly, enter the same title for "Associated Clinic." You will then be able to type in that "Associated Clinic" name in the email box.


To recall a saved email address or email group, start typing in the recipient or associated clinic into the box below.

EMAIL REGISTRATION *(continued)*

e) Recognized contacts will be displayed for you to select:

 Selecting the building icon allows you to email a distribution list of all contacts associated with that clinic.

 Selecting the envelope icon allows you to email an individual contact.

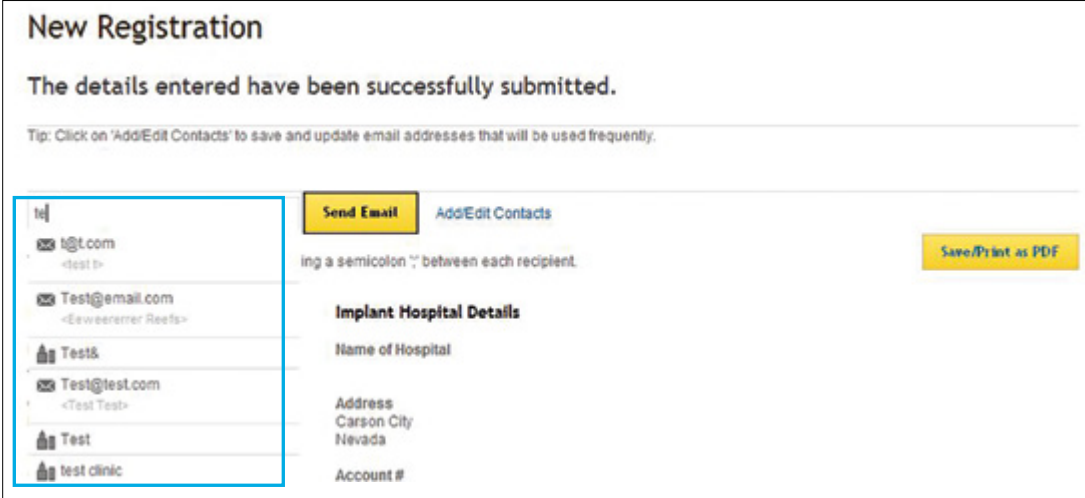

New Registration

The details entered have been successfully submitted.

Tip: Click on 'Add/Edit Contacts' to save and update email addresses that will be used frequently.

Send Email **Add/Edit Contacts** **Save/Print as PDF**

ing a semicolon ";" between each recipient.

Implant Hospital Details

Name of Hospital

Address
Carson City
Nevada

Account #

test.com
<test@>

Test@email.com
<Eewee@erret Reets>


Test&

Test@test.com
<Test Test>

Test

test clinic

To leave the system, select **Log Out**. To switch users, click on your name at the top right of the screen and select the new user.

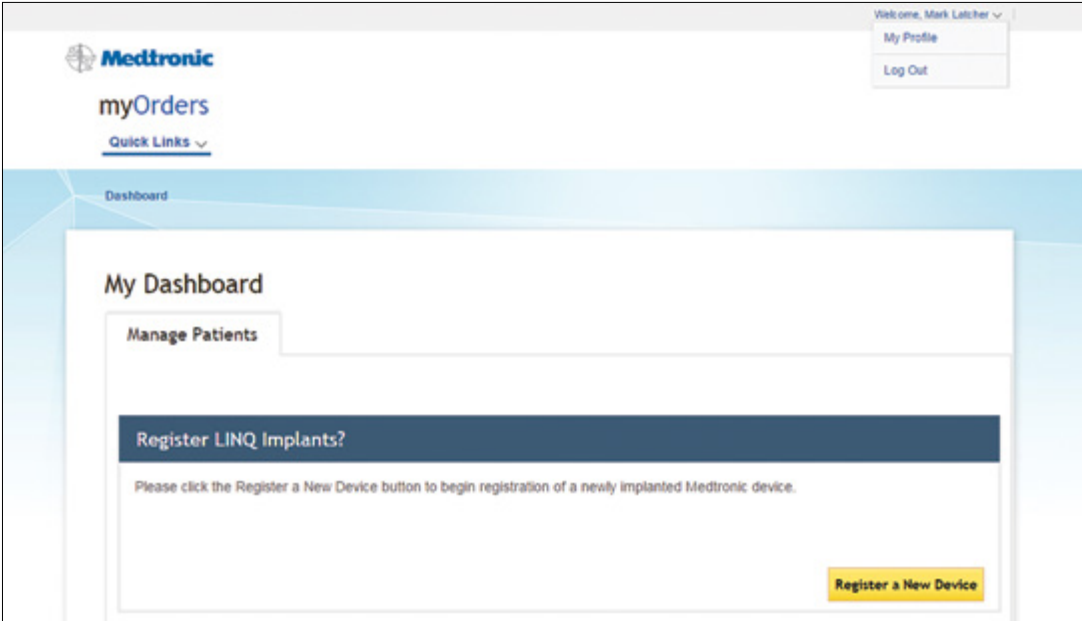

Medtronic
myOrders
Quick Links

Welcome, Mark Latcher

My Profile
Log Out

Dashboard

My Dashboard

Manage Patients

Register LINQ Implants?

Please click the Register a New Device button to begin registration of a newly implanted Medtronic device.

Register a New Device

Note: If a correction is needed to a previously submitted registration, please contact the myOrders Support team: 1 (877) 527-3426.

The record will then be adjusted in the Medtronic device and patient tracking database.

The Medtronic MyCareLink Patient Monitor and the Medtronic CareLink Network are indicated for use in the transfer of patient data from Medtronic implantable cardiac devices. These products are not a substitute for appropriate medical attention in the event of an emergency. Data availability and alert notifications are subject to Internet connectivity and access, and service availability. The MyCareLink Patient Monitor must be on and in range of the device. Alert notifications are not intended to be used as the sole basis for making decisions about patient medical care.

Brief Statement

Reveal LINQ™ LNQ11 Insertable Cardiac Monitor and Patient Assistant

Indications: Reveal LINQ LNQ11 Insertable Cardiac Monitor

The Reveal LINQ Insertable Cardiac Monitor is an implantable patient-activated and automatically-activated monitoring system that records subcutaneous ECG and is indicated in the following cases:

- patients with clinical syndromes or situations at increased risk of cardiac arrhythmias
- patients who experience transient symptoms such as dizziness, palpitation, syncope, and chest pain, that may suggest a cardiac arrhythmia

This device has not been specifically tested for pediatric use.

Patient Assistant: The Patient Assistant is intended for unsupervised patient use away from a hospital or clinic. The Patient Assistant activates the data management feature in the Reveal Insertable Cardiac Monitor to initiate recording of cardiac event data in the implanted device memory.

Contraindications: There are no known contraindications for the implant of the Reveal LINQ Insertable Cardiac Monitor. However, the patient's particular medical condition may dictate whether or not a subcutaneous, chronically implanted device can be tolerated.

Warnings/Precautions: Reveal LINQ LNQ11 Insertable Cardiac Monitor

Patients with the Reveal LINQ Insertable Cardiac Monitor should avoid sources of diathermy, high sources of radiation, electrosurgical cautery, external defibrillation, lithotripsy, therapeutic ultrasound, and radiofrequency ablation to avoid electrical reset of the device, and/or inappropriate sensing as described in the Medical procedure and EMI precautions manual. MRI scans should be performed only in a specified MR environment under specified conditions as described in the Reveal LINQ MRI Technical Manual.

Patient Assistant: Operation of the Patient Assistant near sources of electromagnetic interference, such as cellular phones, computer monitors, etc., may adversely affect the performance of this device.

Potential Complications: Potential complications include, but are not limited to, device rejection phenomena (including local tissue reaction), device migration, infection, and erosion through the skin.

See the device manual for detailed information regarding the implant procedure, indications, contraindications, warnings, precautions, and potential complications/adverse events. For further information, please call Medtronic at 1 (800) 328-2518 and/or consult Medtronic's website at www.medtronic.com.

Medtronic MyCareLink™ Patient Monitor, Medtronic CareLink™ Network and CareLink™ Mobile Application

Intended Use

The Medtronic MyCareLink Patient Monitor and CareLink® Network are indicated for use in the transfer of patient data from some Medtronic implantable cardiac devices based on physician instructions and as described in the product manual. The CareLink Mobile Application is intended to provide current CareLink Network customers access to CareLink Network data via a mobile device for their convenience. The CareLink Mobile Application is not replacing the full workstation, but can be used to review patient data when a physician does not have access to a workstation. These products are not a substitute for appropriate medical attention in the event of an emergency and should only be used as directed by a physician. CareLink Network availability and mobile device accessibility may be unavailable at times due to maintenance or updates, or due to coverage being unavailable in your area. Mobile device access to the Internet is required and subject to coverage availability. Standard text message rates apply.

Contraindications

There are no known contraindications.

Warnings and Precautions

The MyCareLink Patient Monitor must only be used for interrogating compatible Medtronic implantable devices.

See the device manuals for detailed information regarding the implant procedure, indications, contraindications, warnings, precautions, and potential complications/adverse events. For further information, please call Medtronic at 1 (800) 328-2518 and/or consult Medtronic's website at www.medtronic.com.

Caution: Federal law (USA) restricts these devices to sale by or on the order of a physician.



Medtronic
710 Medtronic Parkway
Minneapolis, MN 55432-5604
USA
Tel: (763) 514-4000
Fax: (763) 514-4879

medtronic.com

Toll-free: 1 (800) 328-2518
(24-hour technical support for
physicians and medical professionals)

UC201405279d EN © Medtronic 2015.
Minneapolis, MN. All Rights Reserved.
Printed in USA. 09/2015

Medtronic