

Jul

Department of Forensic Science
Breath Alcohol Section
Instrument Location History
1/1/1990 To 9/22/2014

Instrument Serial Number: 010420

As of 22-Sep-14

Start Date	End Date	Agency Name
19-Sep-14		DFS Central Lab
18-Apr-14	19-Sep-14	South Hill PD
08-Apr-14	18-Apr-14	DFS Central Lab
24-Sep-13	08-Apr-14	Galax PD
21-Dec-12	24-Sep-13	DFS Central Lab
19-Oct-12	21-Dec-12	Virginia Peninsula Regional Jail
14-Mar-11	19-Oct-12	DFS Central Lab
20-Jan-10	14-Mar-11	Arlington County PD
30-Sep-09	20-Jan-10	DFS Central Lab
21-Nov-08	30-Sep-09	Orange County SO
27-May-08	21-Nov-08	DFS Central Lab

rd

INTOX EC/IR II Quality Assurance Worksheet

Instrument Serial Number 010420 Worksheet Start Date 9/19/2014
Location South Hill Police Department
Address 103 S Brunswick Ave South Hill VA 23970
DFS Technician Sarah Dersch License No. 24178

☐ Laboratory ☒ On-Site

Site Specification: No detrimental environmental conditions exist. ☒

Instrument Barometer (mm HG) 755 Reference Barometer (mm HG) 756
Reference Barometer(RB)Serial # 009111 RB Calibration Due 5/19/2015

Measurement Assurance Check

Standard (sea level)	PA Target	minimum	maximum	Sample 1	0.300
0.300	0.298	0.289	0.306	Sample 2	0.299
Precision		sample min	sample max	Sample 3	0.299
0.001		0.299	0.300		

Standard (sea level)	PA Target	minimum	maximum	Sample 1	0.099
0.100	0.099	0.096	0.102	Sample 2	0.099
Precision		sample min	sample max	Sample 3	0.099
0		0.099	0.099		

Dry gas standard Lot No. (with tank no.) AG316301-26

☐ Replaced dry gas standard (+O-ring)

☐ Installed at Location

☒ Removed to DFS-Central

Supplies
Mouthpieces
Certificates of Analysis
Operator Worksheet
Other:



Notes:

Instrument Serial Number

010420

Certification Date

☐ Calibrated☐ Certified☒ Measurement Assurance Check☒ Instrument Test☐ Troubleshooting/Maintenance Worksheet Completed

(Successful completion denotes satisfactory condition of the item.)

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.250		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.150		0.000	0.000	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	


Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.080		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

Standard (sea level)	PA Target	minimum	maximum	Sample 1
0.020		-0.003	0.003	Sample 2
Precision		sample min	sample max	Sample 3
0		0.000	0.000	

All measurements are in g/210L

Estimation of Uncertainty of Measurement and traceability records are located within the Breath Alcohol Section


DFS Technician



Date

9/22/14

Issuing Analyst

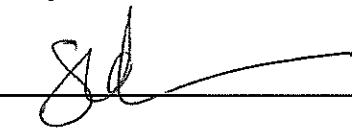

Date

9/22/14






COMMONWEALTH OF VIRGINIA
DEPARTMENT OF FORENSIC SCIENCE

CERTIFICATE OF BLOOD ALCOHOL ANALYSIS
AS DETERMINED BY A CHEMICAL TEST OF THE ACCUSED'S BREATH

NAME OF ACCUSED INSTRUMENT, TEST,	NAME OF COURT DFS
-------------------------------------------------	---------------------------------

BREATH ANALYSIS

SAMPLE EXAMINED AND TEST CONDUCTED BY DERSCHE, SARAH, E		AGENCY DFS Central Lab
DFS LICENSE NUMBER 24178	LICENSE EXPIRES 10/01/2014	DATE TEST CONDUCTED 09/19/2014
TEST EQUIPMENT NUMBER 010420		

RESULTS: TIME SAMPLE TAKEN 11:07 EDT

SAMPLE'S ALCOHOL CONTENT 0.00 GRAMS PER 210 LITERS OF BREATH

ATTEST:

I CERTIFY THAT THE ABOVE IS AN ACCURATE RECORD OF THE TEST CONDUCTED; THAT THE TEST WAS CONDUCTED WITH THE TYPE OF EQUIPMENT AND IN ACCORDANCE WITH THE METHODS APPROVED BY THE DEPARTMENT OF FORENSIC SCIENCE; THAT THE TEST WAS CONDUCTED IN ACCORDANCE WITH THE DEPARTMENT'S SPECIFICATIONS; THAT PRIOR TO ADMINISTRATION OF THE TEST THE ACCUSED WAS ADVISED OF HIS RIGHT TO OBSERVE THE PROCESS AND SEE THE BLOOD ALCOHOL READING ON THE EQUIPMENT USED TO PERFORM THE BREATH TEST, AND THAT I POSSESS A VALID LICENSE TO CONDUCT SUCH TEST, GIVEN UNDER MY HAND THIS _____ DAY OF _____, 20_____.

BREATH TEST OPERATOR

☐ I HAVE RECEIVED A COPY OF THIS CERTIFICATE OF ANALYSIS _____ SUBJECT'S SIGNATURE

☐ SUBJECT REFUSED TO SIGN FOR COPY OF CERTIFICATE OF ANALYSIS _____ OPERATOR'S SIGNATURE



IntoxNet MIS Report

Report Generated 19 Sep 2014 at 11:34

TLW
red

Test Results

Instrument Serial Number 010420

Test # 001192 Subject Test

Test Location 1 Department of
Test Date 19 Sep 2014

Test Location 2 Forensic Science
Test Time 11:00
Remote/Local Local

Test Location 3
System Check Passed

Operator's Last Name DERSCH
Agency DFS Central Lab

Operator's First Name SARAH

Operator's Middle Initial E
License Number 24178

Card Serial Number 124178

Effective Date 10/01/2012

Expiration Date 10/01/2014

Subject's Last Name INSTRUMENT

Subject's First Name TEST

Subject's Middle Initial

Subject's Date of Birth 00/00/0000

Subject's Sex Male

Driver's License Number

Driver's License Expiration 00/00/0000

Driver's License State

Court Name DFS

End Date 19 Sep 2014 End Time 11:08

Result Time 11:07

Result Date 19 Sep 2014 Result 0.00

Data Type DIAG

Sample Value Pass

Sample Time 11:01

Data Type BLK

Sample Value 0.000

Sample Time 11:01

Data Type CHK

Sample Value 0.100

Sample Time 11:02

Data Type BLK

Sample Value 0.000

Sample Time 11:03

Data Type SUBJ

Sample Value 0.000

Sample Time 11:04

Data Type BLK

Sample Value 0.000

Sample Time 11:05

Data Type SUBJ

Sample Value 0.000

Sample Time 11:07

Data Type BLK

Sample Value 0.000

Sample Time 11:08

Standard Type Dry Gas Std

Standard Value 0.099

Standard Lot Number AG316301-26

Standard Expiration Date 06/12/2015

Tank Pressure 296

Barometric Pressure 755 mmHg

Blow Sample Number 1 Blow Duration 3.69 sec

Blow Volume 1806 cc End-of-Blow Time 11:04

Blow Sample Number 2 Blow Duration 4.06 sec

Blow Volume 1939 cc End-of-Blow Time 11:07

Tamper Evident Stamp a545d742

Test Status Code 0

Test Status Success

Intox EC/IR-II: Accuracy Check

ser

Department of Forensic Science

Serial Number: 010420 Test Number: 1193

Test Date: 09/19/2014 Test Time: 11:10 EDT

Dry Gas Target: 0.099

Lot Number: AG316301-26 Exp Date: 06/12/2015

Tank Pressure: 296 psi Barometric Pressure: 755 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	11:11
CHK	0.099	11:12
BLK	0.000	11:13
CHK	0.099	11:14
BLK	0.000	11:15
CHK	0.099	11:16

Test Status: *Success*

Calibration CRC: DA50A6BD

Intox EC/IR-II: Accuracy Check

sd

Department of Forensic Science

Serial Number: 010420 Test Number: 1194

Test Date: 09/19/2014 Test Time: 11:19 EDT

Dry Gas Target: 0.298

Lot Number: AG421201-04 Exp Date: 07/31/2016

Tank Pressure: 409 psi Barometric Pressure: 755 mmHg

System Check: *Passed*

Test	g/210L	Time
BLK	0.000	11:20
CHK	0.300	11:21
BLK	0.000	11:22
CHK	0.299	11:23
BLK	0.000	11:24
CHK	0.299	11:25

Test Status: *Success*

Calibration CRC: DA50A6BD