

Immunology
Line

Catalogue
Price List

2012



Via Torino, 12 - 22070 Fenegrò (CO)



IMMUNOLOGY LINE

CATALOGUE - PRICE LIST 2012

New Scientific Company S.r.l.

Via Torino, 12
I - 22070 Fenegrò (CO)
Phone (+39) 031 938 132
Fax (+39) 031 352 04 09
<http://www.newscientific.com>
e-mail: nscit@newscientific.com

Spain

New Scientific Company España S.L.
c/ Valencia, 558
E - 08026 Barcelona
Phone (+34) 93 244 82 94
Fax (+34) 93 244 82 95
e-mail: nsce@newscientific.com

INDEX

General	5
Company	5
Acknowledgement	5
Study Commissions on Bence Jones Proteins and Free Light Chains	5
Free Light Chains line - Presentation	7
Introduction	9
Uses	9
Test Values	10
Applications	11
Characteristics of the Method	11
Kits Available	12
Kit Characteristics	12
Protocol Operative in Urine - Example	13
Bibliography	14
Free Light Chains line - Catalogue /Price List	17
ImmunoTurbidimetry - ITA	19
ImmunoTurbidimetry - ITAN	20
ImmunoNephelometry - Immage	21
ImmunoNephelometry - BN series	22
Calibrators - Prediluted Calibrator Sets - Controls	23
Other Proteins - Catalogue/Price List	25
ImmunoNephelometry - Immage	27
ImmunoNephelometry - BN series	29
Calibrators - Prediluted Calibrator Sets - Controls	30

GENERAL

Company

The New Scientific Company, founded in 1981, operates in the "Clinical Chemistry: Analysis of Protein".

The NSC produces, distributes and provides an after-sales service for high quality products, through specific internal professional skills, innovative and at times exclusive, with an attractive price-quality ratio.

In addition to its own products, the NSC distributes products selected from the best available in the market.

Innovative and high quality such products are carefully chosen, rigorous and continuous quality control is undertaken, and a fast, qualified service in the applied procedure and in the operative protocol use are adopted.

Both promotion and service are in the hands of staff with an excellent level of competence and long experience.

Acknowledgement

In 1990 the NSC was awarded "Il Premio per l'Innovazione Tecnologica della Camera di Comercio di Milano" ("The Milan Chamber of Commerce Award for Technological Innovation") for its activity in research in the determination of Free Light Chains.

Study Commissions on Bence Jones Proteins and Free Light Chains

The NSC is organiser and co-ordinator of the following commissions on this subject:

- *Inter-Regional Study Commission "Forlì"*

Scientific Secretary: **Gualtiero Pallotti**, Pierantoni Hospital, Forlì

Set up: 1993; 10 meetings, the last of which was on 16 June 2000

Participants: about 30 Laboratories.

- *Joined Commission "SIBIOC – AIPAC – SIMEL, Liguria Sections"*

Scientific Secretary:

- **Liliana Burlando**, ex Galliera Hospital, Genoa

- Giovanna Zaninetta, S. Martino Hospital, Genoa.

Set up: 1997; 4 meetings, the last of which was on 22 June 2000

Participants: 14 Laboratories.

■ ***Study Commission "Lazio"***

Scientific Secretary: ***Maria Teresa Muratore*** – Civil Hospital – Viterbo

First meeting: 10 April 2001 – Participants: 11 Laboratories.

■ ***Study Commission "Toscana-Umbria"***

Scientific Secretary: ***Enzida Piazza*** – Careggi Hospital – Florence

First meeting: 24 may 2001 – Participants: 17 Laboratories.

The Commission work is orientated towards the standardisation of various aspects of Bence Jones research and gave us the **Bence Jones controls** named:

- *Bence Jones kappa "Lavagna" Control*
- *Bence Jones lambda "Bellaria" Control*

available from the New Scientific Company.

The Commissions were invited to present the results of their work at the CEFAR - SIBioC meeting "Le Proteine: dal Laboratorio alla clinica" ("Proteins: from the Laboratory to the Clinic") – the most important national meeting on this subject – for the first time in 1999 in Desenzano, then in 2000 in Fiuggi and the latest in 2001 in Castrocaro.

FREE LIGHT CHAINS LINE PRESENTATION

Introduction

This line is exclusive to the NSC and is the result of specific internal work. The objective of the kits is for the qualitative and/or quantitative determination of Free Light Chains in unconcentrated urine and cerebrospinal fluid.

The method is based upon the reaction of ImmunoPrecipitation in liquid phase with specific adsorbed antisera anti Free Light Chain – "Hidden" Determinants.

The turbidity produced by the reaction can be:

- evaluated visually with suitable lighting:
 - non-instrumental qualitative determination
The turbidity produced by the specimen is compared to that of the "Sample Blank" and to that of the calibrators with the dilution chosen as the minimum concentration retained significant (cut off).
 - measured instrumentally: turbidimetry or nephelometry:
 - instrumental qualitative determination:
The signal produced by the specimen is compared to that produced by the Calibrators with the dilution chosen as the minimum concentration retained significant (cut off).
 - quantitative determination:
The specimen signal is interpolated into the curves obtained with the Calibrators.

Free Light Chains in Blood

By using the kits on serum and plasma, with the same application as that of urine, technically and analytically excellent results are obtained (15); however, we must emphasise that the clinical significance of the determination of the concentration of Free Light Chains in blood is currently being studied and defined (23). Thus this brochure refers only to urine and cerebrospinal fluid.

Uses

Determination of Free Light Chains has many uses:

Monoclonal Free Light Chains in urine - Bence Jones Proteinuria (BJP)

- Protocol in the case of:
 - clinically-suspected immunoproliferative disease such as:
 - Waldenström's Macroglobulinemia, Multiple Myeloma, Chronic Lymphatic

- Leukaemia, primitive Amyloidosis etc.
- Serum Electrophoresis which highlights a new monoclonal band.
- laboratory data which show suspected micromolecular myeloma.
- **Follow-up in the case of:**
 - immunoproliferative disease.
 - patients with monoclonal band in serum electrophoresis but without diagnosis of immunoproliferative disease (MGUS).
- **Pre-contrastographic tests:**
The contraindications in the use of contrast media by injection include "Waldenström's Macroglobulinemia" and "Multiple Myeloma".
In order to exclude the fact that the patient may be affected by "multiple myeloma", electrophoresis of the serum protein is not sufficient but it is necessary to carry out detection of Bence Jones Protein in urine. In fact, in cases of micromolecular myeloma electrophoresis of the serum frequently shows no significant or specific alterations.

Polyclonal Free Light Chains in Urine

- **Protocol in research for hyperimmune diseases such as:**
Lupus Erythematosus, Rheumatoid Arthritis, Secondary Amyloidosis, etc.
- **Protocol in research for functionality of proximal tubule**
Here, the Free Light Chains have the same significance as that of other microglobulins.

Free Light Chains in Cerebrospinal Fluid

Protocol for research for the diagnosis and control of diseases of the Central Nervous system, such as Multiple Sclerosis and Other Inflammatory Diseases.

Test Values

The value of the test will depend upon the problem:

- **Bence Jones Protein:**
 - **diagnosis:** the test has two values:
 - *qualitative screening*
 - Regardless of the reason for the research, the value of the test is, above all, for qualitative screening, since the monoclonality will in any case have to be verified with Electrophoresis or

- ImmunoFixation.
- *quantitative indication*
Quantitative determination, even though it has its limits, is useful for:
 - providing a guidance as to how much to concentrate the sample for further research
 - providing a starting point for evolution control.
- **follow-up:** the test has a predominantly quantitative significance.
- **Polyclonal Free Light Chains in Urine:**
the test has a predominantly quantitative significance.
- **Free Light Chain in Cerebrospinal fluid:**
the test has a predominantly quantitative significance.

Applications

The application of the test can be outlined thus:

- **Qualitative:**
Screening Test under "Bence Jones Protein" research protocol.
- **Quantitative:**
 - "Bence Jones Protein" – Monoclonal Free Light Chains in urine.
 - Polyclonal Free Light Chains in urine.
 - Free Light Chains in Cerebrospinal fluid

Characteristics of the Method

- **Specificity**
Adsorbed antisera are utilised and these react exclusively with the "hidden" determinants of Free Light Chains.
The specificity is demonstrated by the absence of specific reaction when a normal human serum is used as sample.
- **Unconcentrated Sample**
An "unconcentrated" sample with no prior treatment is used.
- **Sensitivity**
It is evaluated for "internal standardisation" and the results are:
 - kit with normal sensitivity : 0.5 mg/dl
 - kit with high sensitivity (HS) : 0.2 mg/dl

- **Automation**

Kits and operating procedures are available for:

- automatic analyzers of clinical chemistry
- "BN series" (BNA, BNII, BN ProSpec) Siemens (ex Behring) nephelometry and similar.
- "Immage" Beckman nephelometry, and similar.

- **Quantitative Dosage**

The kit calibrators allow construction of the calibrator curves in order to achieve quantitative determination.

Kits Available

The following types of kit are available:

- *kit containing mixed reagent anti Free Light Chains kappa+lambda*
 - normal sensitivity : up to 0.5 mg/dl
- *kit containing separate reagents: anti Free Light Chains kappa and lambda*
 - normal sensitivity : up to 0.5 mg/dl
 - high sensitivity (HS): up to 0.2 mg/dl

The following are available for each type:

- *ITA kits – ImmunoTurbidimetry Kit:*
 - instrumental: Photometers and Automatic Photometric Analyzers.
- *BN series kits – ImmunoNephelometry: "BN series"(BNA,BNII, BN ProSpec) Siemens (ex Dade Behring) Nephelometry, and similar.*
- *Immagine kits – ImmunoNephelometry: "Immagine" Beckman Coulter Nephelometry, and similar.*

Kit Characteristics

- **Type:** all components are liquid and ready to use.


- **Preservative:** Sodium Azide < 0,1% (w/v).

- **Stability:** over 1 year at 2 - 8°C.

All kits come complete with Calibrators–Controls. Accessory reagents are separate.

Protocol Operative in Urine - Example

The Operative Protocol which follows is an example of the utilization of the FLC kit in Urine in its initial diagnostic approach.

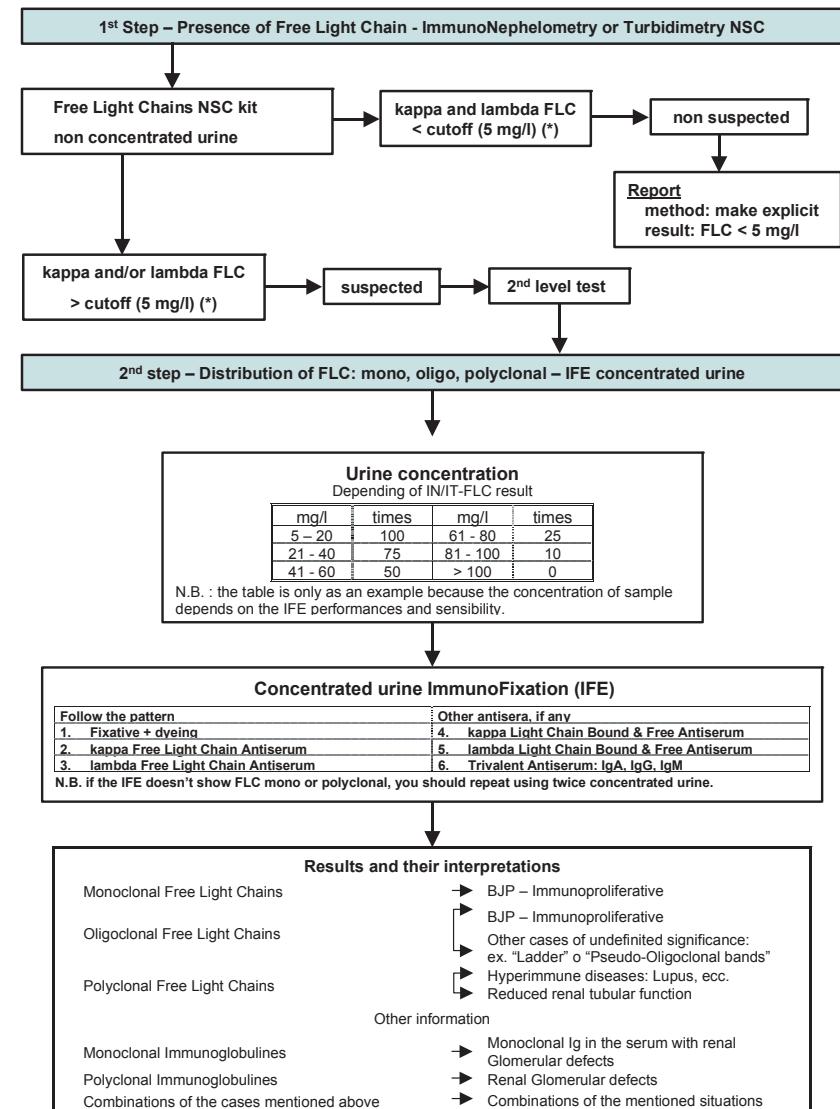

(*) or as defined by user

Bibliography

Note: The articles, posters and Meeting presentations are available from New Scientific Company.

- 1 Abate L, Martelli M, Zannini R.
Proteinuria di Bence Jones: sperimentazione di un nuovo metodo immunoturbidimetrico per la determinazione delle Catene Leggere Libere nelle urine non concentrate
Biochimica Clinica, 12, 1988, p.: 1451,1457
- 2 Massaro L.
Metodo Immunoturbidimetrico - Immunonefelometrico per la Determinazione delle Catene Leggere Libere nelle Urine
Riunione: SIBIOC / PROTEINE - Asti, 17 - 19 October 1989
- 3 Migliorati T.
Uso della prova di Precipitazione in Provetta per Immunoglobuline Urinarie o loro frammenti presenti in Gamopetale Monoclonali
Biochimica Clinica, 13, 1989, p.: 1237-1240
- 4 Massaro L.
Lettera a F. Aguzzi
L'Angolo dell'Elettroforesi - Biochimica Clinica, 14, 1990, p.: 70-72
- 5 Alecci A, Brandini A.
Amiloidosi AL o Amiloidosi AH ?
Biochimica Clinica, 14, 1990, p.: 471-472
- 6 Martelli M, Zannini R.
Proposal of a working model for research into Bence Jones Proteinuria
Poster - Proteins ecc - Padova, 16-17 Marzo 1991
- 7 Valentini D, Lenzi MC, Mammini P.
Ricerca qualitativa e quantitativa delle Proteine di Bence Jones
Gior. It. Chim. Clin., 16, 6, 1991, p.: 403-407
- 8 Massaro L.
Catene Leggere Libere "pseudo-oligoclonali" in urine. Riflessioni indotte da recenti lavori
Lettera a F. Aguzzi - L'Angolo dell'Elettroforesi - Biochimica Clinica, 16, 1992, p.: 1213-1215
- 9 Milanesi MG et altri
Commissione InterRegionale "Forlì" su Proteine di Bence Jones e Catene Leggere Libere
Valutazione Multicentrica di Metodi e protocolli per le Catene Leggere Libere e Proteine di Bence Jones in urine – Primi Risultati
Biochimica Clinica, 19, 1995, p.: 410-425

- 10 Procaccianti G, Cucci A, Scaringi R, Massaro L.
A New ImmunoNephelometric method for Free Light Chains assay in the Cerebrospinal Fluid of neurological patients: preliminary results
European Charcot Foundation – Symposium "Body fluid markers for course and activity of disease in Multiple Sclerosis" – Madrid, 2 – 4 October, 1997
- 11 Massaro L, Scaringi R.
Catene Leggere Libere e Proteine di Bence Jones – Review V Edizione, Ottobre 1999
Edito da New Scientific Company
- 12 Gruppi di studio "Forlì" e "Liguria" su "Proteine di Bence Jones e Catene Leggere Libere"
Presenta: Tizzanini W. – *Laboratorio Analisi – Azienda Policlinico – Modena*
Valutazione Multicentrica di Metodi commerciali di routine per la ricerca delle Proteine di Bence Jones nelle urine
Meeting SIBIOC - CEFAR "Le Proteine: dal Laboratorio alla Clinica" – VIII edizione – Desenzano, 1999
- 13 Gruppi di studio "Forlì" e "Liguria" su "Proteine di Bence Jones e Catene Leggere Libere"
Presenta: Tizzanini W. - *Laboratorio Analisi – Azienda Policlinico – Modena*
Valutazione Multicentrica di Metodi commerciali di routine per la ricerca delle Proteine di Bence Jones nelle urine
Meeting SIBIOC - CEFAR "Le Proteine: dal Laboratorio alla Clinica" – IX edizione – Fiuggi, 2000
- 14 Regeniter A^a, Siede WH. ^b
(a) Presenting autor: Central Laboratory, Kantonsspital Basel, Switzerland
(b) Author for correspondence: Central Laboratory, Klinikum Lippe-Lemgo, Lemgo, Germany
Evaluation and Presentation of laboratory Results in Patients suspected of a monoclonal Gammopathy: The value of free light Chains in Bence Jones Testing (abstract)
Meeting SIBIOC - CEFAR "Proteins: from the Laboratory to the Clinic" - X edition - Castrocaro 2001
- 15 Quinzanini M.
Servizio di Reumatologia Immunologia ed Allergologia – Azienda Ospedaliera "Spedali Civili" di Brescia
ImmunoNephelometric Determination of Free Light Chains of Immunoglobulins in Urine for the Detection of Bence Jones Proteins, and Comparison with Immunofixation
Meeting SIBIOC - CEFAR "Proteins: from the Laboratory to the Clinic" - X edition - Castrocaro 2001
- 16 Gruppi di Studio su "Catene Leggere Libere e Proteine di Bence Jones": Forlì, Liguria, Lazio, Toscana-Umbria
Presenta: Tizzanini W. - *Laboratorio Analisi – Azienda Policlinico – Modena*
Multi-Centre Evaluation of Routine Commercial Methods for the Detection of Bence Jones Proteins in Urine – 2001 Results
Meeting SIBIOC - CEFAR "Proteins: from the Laboratory to the Clinic" - X edition - Castrocaro 2001
- 17 Burlando L.
Già Laboratorio Analisi – Ospedale Galliera – Genova
The Detection of Bence Jones Proteins - A Review from the Records of the Ospedali Galliera, Genoa
Meeting SIBIOC - CEFAR "Proteins: from the Laboratory to the Clinic" - X edition - Castrocaro 2001

18

Viedma JA.
Hospital General & Universitario – Elche (Alicante), Spain

Monoclonal and Polyclonal Immunoglobulin Free Light Chains (FLC) detection in urine

Meeting SIBioC - CEFAR "Proteins: from the Laboratory to the Clinic" - X edition - Castrocaro 2001

19

Siede WH^a, Regeniter A.^b
(a) Presenting Author: Central Laboratory, Klinikum Lippe-Lemgo, Lemgo, Germany
(b) Author for correspondence: Central Laboratory, Kantonsspital Basel, Switzerland

Proteinuria – Diagnostics and Interpretation with Marker Proteins - Computerising Processing and report ("MDI-LabLink")

Meeting SIBioC - CEFAR "Proteins: from the Laboratory to the Clinic" - X edition - Castrocaro 2001

20

Quiñones-Torrelo C, Del Valle-Pérez R, González-Ovelar M, Jarabo-Bueno MM, Díaz-Ruiz M, Montagud-Palau A, González-Monleón L, Marco-López P.

Immunochemistry Section. Clinical Analysis Department. "Dr. Peset" University Hospital. Valencia (Spain)

Evaluation of an ImmunoFixation Electrophoresis selective method for Bence Jones Proteinuria Identification

EUROMEDLAB Barcelona 2003 - 15th European Congress of Clinical Chemistry and Laboratory Medicine

22nd National Congress of the Spanish Society of Clinical Biochemistry and Molecular Pathology

21

García-Vitoria, M.; Cortina, A.; Iglesias, N.; Hernández, M.; García-Guantes, E.; Besalú, C.; Galimany, R.; Rodrigo, MJ.

Laboratoriis Clínics, Hospital Vall d'Hebron, Barcelona. Spain

ImmunoNephelometric Determination of Free Light Chains in Urine as Screening for the Detection of Bence Jones Proteinuria

EUROMEDLAB Barcelona 2003 - 15th European Congress of Clinical Chemistry and Laboratory Medicine

22nd National Congress of the Spanish Society of Clinical Biochemistry and Molecular Pathology

22

Quinlanini M.
Department of Rheumatology, Immunology & Allergology, Azienda Ospedaliera "Spedali Civili", Brescia, Italy

ImmunoNephelometric Determination of Free Light Chains of Immunoglobulins in Urine for the Detection of Bence Jones Proteins, and Comparison with Immunofixation

EUROMEDLAB Barcelona 2003 - 15th European Congress of Clinical Chemistry and Laboratory Medicine

22nd National Congress of the Spanish Society of Clinical Biochemistry and Molecular Pathology

23

Tate JR¹, Gill D, Cobcroft R², Hickmann P²

¹Chemical Pathology and ²Haematology Departments, Queensland Health Pathology Service, Princess Alexandra Hospital, Woolloongabba, Queensland, Australia

Practical Consideration for the Measurement of Free Light Chains in serum

Clinical Chemistry 49;6 1252 – 1257 (2003)

FREE LIGHT CHAINS LINE

CATALOGUE - PRICE LIST

ImmunoTurbidimetry**ITA**

These kits are for the determination of Free Light Chains with the ImmunoTurbidimetric method on automatic biochemistry analyzers.

<i>Product</i>	<i>Pack</i>	<i>Code</i>	<i>Euro</i>
Kits			

Free Light Chain Kit Separate Reagents	70 + 70 tests(*)	K.ITA.FR.K.FRL	1.006,00
---	---------------------	-----------------------	-----------------

The kit contains:

- Antiserum Reagent anti:
 - Free Light Chains kappa 1 x 18 ml R.ITA.FR.K
 - Free Light Chains lambda 1 x 18 ml R.ITA.FRL
- Calibrators - Controls:
 - Free Light Chains kappa 1 x 1 ml W.UPC.FR.K
 - Free Light Chains lambda 1 x 1 ml W.UPC.FRL

Free Light Chain Kit "Mixed" Reagent	70 tests(*)	K.ITA.FKL	960,00
---	-------------	------------------	---------------

The kit contains:

- Antiserum reagent "Mixed" anti:
 - Free Light Chains kappa+lambda 1 x 18 ml R.ITA.FKL
- Calibrators - Controls:
 - Free Light Chains kappa+lambda 1 x 1 ml W.UPC.FKL

Free Light Chains Kit High Sensitivity (HS)	40 + 40 tests(*)	K.ITA.FR.K.FRL.HS	on request
--	---------------------	--------------------------	-------------------

The kit contains:

- Antiserum Reagent HS anti:
 - Free Light Chains kappa 1 x 10 ml R.ITA.FR.K.HS
 - Free Light Chains lambda 1 x 10 ml R.ITA.FRL.HS
- Calibrators - Controls:
 - Free Light Chains kappa 1 x 1 ml W.UPC.FR.K
 - Free Light Chains lambda 1 x 1 ml W.UPC.FRL

Accessory Reagents

Reagent Without Antiserum	1 x 20 ml	R.ITA.RWA	207,00
Sample Diluent	1 x 20 ml	R.ITA.SDA	207,00

Calibrators - Prediluted Calibrator Sets - Controls

See relative chapter, page 23

Key (*) the number of tests is evaluated utilizing 250ml/test

ImmunoTurbidimetry ITAN

These kits are for the determination of Free Light Chains with the ImmunoTurbidimetric method on [some automatic biochemistry analyzers](#).

Product	Pack	Code	Euro
---------	------	------	------

Kits

Free Light Chain Kit Separate Reagents	100+100 tests(*)	K.ITAN.FR.K.FRL	1.422,00
---	------------------	------------------------	-----------------

The kit contains:

- Antiserum Reagent anti:
 - Free Light Chains kappa 1 x 15 ml R.ITAN.FR.K
 - Free Light Chains lambda 1 x 15 ml R.ITAN.FRL
- Calibrators - Controls:
 - Free Light Chains kappa 1 x 1 ml W.UPC.FR.K
 - Free Light Chains lambda 1 x 1 ml W.UPC.FRL

Free Light Chain Kit "Mixed" Reagent	100 tests(*)	K.ITAN.FKL	1.422,00
---	--------------	-------------------	-----------------

The kit contains:

- Antiserum reagent "Mixed" anti:
 - Free Light Chains kappa+lambda 1 x 15 ml R.ITAN.FKL
- Calibrators - Controls:
 - Free Light Chains kappa+lambda 1 x 1 ml W.UPC.FKL

Free Light Chains Kit High Sensitivity (HS)	50+50 tests(*)	K.ITAN.FR.K.FRL.HS	on request
--	----------------	---------------------------	-------------------

The kit contains:

- Antiserum Reagent HS anti:
 - Free Light Chains kappa 1 x 7,5 ml R.ITAN.FR.K.HS
 - Free Light Chains lambda 1 x 7,5 ml R.ITAN.FRL.HS
- Calibrators - Controls:
 - Free Light Chains kappa 1 x 1 ml W.UPC.FR.K
 - Free Light Chains lambda 1 x 1 ml W.UPC.FRL

Accessory Reagents

Reagent Without Antiserum	1 x 20 ml	R.ITA.RWA	207,00
Sample Diluent	1 x 20 ml	R.ITA.SDA	207,00

Calibrators - Prediluted Calibrator Sets - Controls

See relative chapter, page 23

Key (*) the number of tests is evaluated utilizing 150ml/test

ImmunoNephelometry IMG

These kits are for the determination of Free Light Chains on "Beckman Coulter" "Immage" Nephelometer.

Product	Pack	Code	Euro
---------	------	------	------

Kits

Free Light Chain Kit Separate Reagents	100 + 100 tests	K.IMG.FR.K.FRL	1.422,00
---	-----------------	-----------------------	-----------------

The kit contains:

- Antiserum Reagent anti:
 - Free Light Chains kappa 1 x 2,4 ml R.IMG.FR.K
 - Free Light Chains lambda 1 x 2,4 ml R.IMG.FRL
- Calibrators - Controls:
 - Free Light Chains kappa 1 x 1 ml W.UPC.FR.K
 - Free Light Chains lambda 1 x 1 ml W.UPC.FRL
- Accessory Reagent "B"
 - for Compartment "B" 1 x 3 ml R.IMG.FLC.B

Free Light Chain Kit "Mixed" Reagent	100 tests	K.IMG.FKL	1.422,00
---	-----------	------------------	-----------------

The kit contains:

- Antiserum reagent "Mixed" anti:
 - Free Light Chains kappa+lambda 1 x 2,4 ml R.IMG.FKL
- Calibrators - Controls:
 - Free Light Chains kappa+lambda 1 x 1 ml W.UPC.FKL
- Accessory Reagent "B"
 - for Compartment "B" 1 x 3 ml R.IMG.FLC.B

Free Light Chains Kit High Sensitivity (HS)	40 + 40 tests	K.IMG.FR.K.FRL.HS	on request
--	---------------	--------------------------	-------------------

The kit contains:

- Antiserum Reagent HS anti:
 - Free Light Chains kappa 1 x 1 ml R.IMG.FR.K.HS
 - Free Light Chains lambda 1 x 1 ml R.IMG.FRL.HS
- Calibrators - Controls:
 - Free Light Chains kappa 1 x 1 ml W.UPC.FR.K
 - Free Light Chains lambda 1 x 1 ml W.UPC.FRL
- Accessory Reagent "B"
 - for Compartment "B" 1 x 3 ml R.IMG.FLC.B

See relative chapter, page 23

ImmunoNephelometry BN **CE**

These kits are for the determination of Free Light Chains on "Siemens" (ex "Dade Behring") "BN™ series" Nephelometers: BNA, BNII, BN ProSpec and similar.

Product	Pack	Code	Euro
---------	------	------	------

Kits

Free Light Chain Kit Separate Reagents 100 + 100 tests **K.BNA.FR.K.FRL** **1.422,00**

The kit contains:

- Antiserum Reagent anti:
 - Free Light Chains kappa 1 x 4 ml R.BNA.FR.K
 - Free Light Chains lambda 1 x 4 ml R.BNA.FRL
- Calibrators - Controls:
 - Free Light Chains kappa 1 x 1 ml W.UPC.FR.K
 - Free Light Chains lambda 1 x 1 ml W.UPC.FRL

Free Light Chain Kit "Mixed" Reagent 100 tests **K.BNA.FKL** **1.422,00**

The kit contains:

- Antiserum reagent "Mixed" anti:
 - Free Light Chains kappa+lambda 1 x 4 ml R.BNA.FKL
- Calibrators - Controls:
 - Free Light Chains kappa+lambda 1 x 1 ml W.UPC.FKL

Free Light Chains Kit High Sensitivity (HS) 40 + 40 tests **K.BNA.FR.K.FRL.HS** **on request**

The kit contains:

- Antiserum Reagent HS anti:
 - Free Light Chains kappa 1 x 2 ml R.BNA.FR.K.HS
 - Free Light Chains lambda 1 x 2 ml R.BNA.FRL.HS
- Calibrators - Controls:
 - Free Light Chains kappa 1 x 1 ml W.UPC.FR.K
 - Free Light Chains lambda 1 x 1 ml W.UPC.FRL

Calibrators - Prediluted Calibrator Sets - Controls

See relative chapter, page 23

Calibrators - Prediluted Calibrator Sets - Controls **CE**

This product line is for use as **Calibrator** and **Controls** in the determination of Free Light Chains carried out with NSC's Free Light Chain kits.

Product	Pack	Code	Euro
---------	------	------	------

Calibrators

Free Light Chain kappa	1 x 1 ml	W.UPC.FR.K	100,00
Free Light Chain lambda	1 x 1 ml	W.UPC.FRL	100,00
Free Light Chain kappa+lambda "mixed"	1 x 1 ml	W.UPC.FKL	100,00

Prediluted Calibrator Sets

Prediluted Calibrators	10 x 1 ml	W.SET.UPC.FR.K.FRL	272,00
Free kappa and free lambda			

▪ Prediluted Calibrator set Free kappa	5 x 1 ml	W.SET.UPC.FR.K	
▪ Prediluted Calibrator set Free lambda	5 x 1 ml	W.SET.UPC.FRL	

Prediluted Calibrators	5 x 1 ml	W.SET.UPC.FKL	137,00
Free kappa + lambda "mixed"			

Controls

Control Free Light Chain kappa	1 x 1 ml	Y.UPR.FR.K	62,00
Control Free Light Chain lambda	1 x 1 ml	Y.UPR.FRL	62,00

Control Free Light Chain kappa-medium value	1 x 3 ml	Y.UPR.FR.K.MV-3	186,00
Control Free Light Chain kappa-low value	1 x 3 ml	Y.UPR.FR.K.LV-3	297,00

Control Free Light Chain lambda-medium value	1 x 3 ml	Y.UPR.FRL.MV-3	186,00
Control Free Light Chain lambda-low value	1 x 3 ml	Y.UPR.FRL.LV-3	297,00

OTHER PROTEINS

CATALOGUE - PRICE LIST

ImmunoNephelometry IMG

These kits are for use on "Beckman Coulter" "Immage" Nephelometer.

Complete Kits and **Separate reagents** are available.

Complete Kits

Product	Pack	Code	Euro
<i>Retinol Binding Protein (RBP) - Serum</i>	100 tests	K.IMG.RBP-S	708,00
<i>The kit contains:</i>			
▪ Antiserum Reagent anti Retinol Binding Protein	1 x 3,5 ml	R.IMG.RBP-S	
▪ Accessory Reagent for Compartment "B"	1 x 1 ml	R.IMG.RBP-B	
▪ Calibrator - Retinol Binding Protein	1 x 1 ml	W.SPC.RBP	
▪ Controls:			
▪ Retinol Binding Protein - serum - Medium value	1 x 1 ml	Y.SPR.RBP.MV	
▪ Retinol Binding Protein - serum - Low value	1 x 1 ml	Y.SPR.RBP.LV	
<i>Retinol Binding Protein (RBP) - Urine</i>	100 tests	K.IMG.RBP-U	847,00
<i>The kit contains:</i>			
▪ Antiserum Reagent anti Retinol Binding Protein	1 x 4,7 ml	R.IMG.RBP-U	
▪ Accessory Reagent for Compartment "B"	1 x 1 ml	R.IMG.RBP-B	
▪ Calibrator - Retinol Binding Protein	1 x 1 ml	W.SPC.RBP	
▪ Controls:			
▪ Retinol Binding Protein - urine - Medium value	1 x 1 ml	Y.UPR.RBP.MV	
▪ Retinol Binding Protein - urine - Low value	1 x 1 ml	Y.UPR.RBP.LV	
<i>Complement C1 (esterase) inhibitor (CEI)</i>	100 tests	K.IMG.CEI	357,00
<i>The kit contains:</i>			
▪ Antiserum Reagent anti C1 (esterase) inhibitor	1 x 2,4 ml	R.IMG.CEI	
▪ Calibrator - Complement System Proteins	1 x 1 ml	W.SPC.CS1	
▪ Controls:			
▪ Complement System Proteins - Medium value	1 x 1 ml	Y.SPR.CS1.MV	
▪ Complement System Proteins - Low value	1 x 1 ml	Y.SPR.CS1.MV	
<i>Complement C1q</i>	100 tests	K.IMG.C1Q	472,00
<i>The kit contains:</i>			
▪ Antiserum Reagent anti C1q	1 x 3,5 ml	R.IMG.C1Q	
▪ Calibrator - Complement System Proteins	1 x 1 ml	W.SPC.CS1	
▪ Controls:			
▪ Complement System Proteins - Medium value	1 x 1 ml	Y.SPR.CS1.MV	
▪ Complement System Proteins - Low value	1 x 1 ml	Y.SPR.CS1.MV	

ImmunoNephelometry **IMG**

Reagent Kits

Product	Pack	Code	Euro
Retinol Binding Protein (RBP) - Serum	100 tests	KR.IMG.RBP-S	503,00

The kit contains:

- Antiserum Reagent anti Retinol Binding Protein 1 x 3,5 ml R.IMG.RBP-S
- Accessory Reagent for Compartment "B" 1 x 1 ml R.IMG.RBP.B

Retinol Binding Protein (RBP) - Urine	100 tests	KR.IMG.RBP-U	669,00
--	-----------	---------------------	---------------

The kit contains:

- Antiserum Reagent anti Retinol Binding Protein 1 x 4,7 ml R.IMG.RBP-U
- Accessory Reagent for Compartment "B" 1 x 1 ml R.IMG.RBP.B

Complement C1 (esterase) inhibitor (CEI)	100 tests	KR.IMG.CEI	130,00
---	-----------	-------------------	---------------

The kit contains:

- Antiserum Reagent anti C1 (esterase) inhibitor 1 x 2,4 ml R.IMG.CEI

Complement C1q	100 tests	KR.IMG.C1Q	239,00
-----------------------	-----------	-------------------	---------------

The kit contains:

- Antiserum Reagent anti C1q 1 x 3,5 ml R.IMG.C1Q

Soluble Transferrin Receptor (sTfR)	160 tests	KR.IMG.STFR	1.543,00
--	-----------	--------------------	-----------------

Calibrators - Prediluted Calibrator Sets - Controls

See relative chapter, page 30

ImmunoNephelometry **BN**



These kits are for use on "Siemens" (ex "Dade Behring") "BN™ series" Nephelometers: **BNA, BN100, BNII, BN ProSpec** and similar.

Complete Kits and Separate reagents are available.

Complete Kits

Product	Pack	Code	Euro
Properdin factor B (GBG) (PFB - C3PA)	100 tests	K.BNA.GBG-2	630,00

The kit contains:

- Antiserum Reagent anti Properdin factor B 1 x 4 ml R.BNA.GBG
- Calibrator - Complement System Proteins 1 x 1 ml W.SPC.CS1
- Controls:
 - Complement System Proteins - Medium value 1 x 1 ml Y.SPR.CS1.MV
 - Complement System Proteins - Low value 1 x 1 ml Y.SPR.CS1.MV

Complement C1q

Complement C1q	50 tests	K.BNA.C1Q	494,00
-----------------------	----------	------------------	---------------

The kit contains:

- Antiserum Reagent anti C1q 1 x 2 ml R.BNA.C1Q
- Calibrator - Complement System Proteins 1 x 1 ml W.SPC.CS1
- Controls:
 - Complement System Proteins - Medium value 1 x 1 ml Y.SPR.CS1.MV
 - Complement System Proteins - Low value 1 x 1 ml Y.SPR.CS1.MV

Reagent Kits

Product	Pack	Code	Euro
Properdin factor B (GBG) (PFB - C3PA)	100 tests	KR.BNA.GBG-2	427,00

The kit contains:

- Antiserum Reagent anti Properdin factor B 1 x 4 ml R.BNA.GBG

Complement C1q

Complement C1q	50 tests	KR.BNA.C1Q	282,00
-----------------------	----------	-------------------	---------------

The kit contains:

- Antiserum Reagent anti C1q 1 x 2 ml R.BNA.C1Q

Calibrators - Prediluted Calibrator Sets - Controls

See relative chapter, page 30

Calibrators - Prediluted Calibrator Sets - Controls**Calibrators**

Product	Pack	Code	Euro
<i>Retinol Binding Protein (RBP) - Siero/Urine</i>	1 x 1 ml	W.SPC.RBP	115,00
<i>Complement System Proteins</i>	1 x 1 ml	W.SPC.CS1	92,00

Prediluted Calibrator Sets

Product	Pack	Code	Euro
<i>Retinol Binding Protein (RBP) - Siero/Urine</i>	5 x 1 ml	W.SET.SPC.RBP	338,00
<i>Complement System Proteins</i>	5 x 1 ml	W.SET.SPC.CS1	271,00
<i>Soluble Transferrin Receptor (sTfR)</i>	6 x 1 ml	W.SET.SPC.STFR	602,00

Controls

Product	Pack	Code	Euro
<i>Retinol Binding Protein (RBP)</i>			
<i>Serum - Medium Value</i>	1 x 1 ml	Y.SPR.RBP.MV	115,00
<i>Serum - Low Value</i>	1 x 1 ml	Y.SPR.RBP.LV	115,00
<i>Urins - Medium Value</i>	1 x 1 ml	Y.UPR.RBP.MV	115,00
<i>Urins Low Value</i>	1 x 1 ml	Y.UPR.RBP.LV	115,00
<i>Complement System Proteins</i>			
<i>Medium Value</i>	1 x 1 ml	Y.SPR.CS1.MV	92,00
<i>Low Value</i>	1 x 1 ml	Y.SPR.CS1.LV	92,00

Retinol Binding Protein (RBP)

<i>Serum - Medium Value</i>	1 x 3 ml	Y.SPR.RBP.MV-3	343,00
<i>Serum - Low Value</i>	1 x 3 ml	Y.SPR.RBP.LV-3	343,00
<i>Urins - Medium Value</i>	1 x 3 ml	Y.UPR.RBP.MV-3	343,00
<i>Urins - Low Value</i>	1 x 3 ml	Y.UPR.RBP.LV-3	343,00

Complement System Proteins

<i>Medium Value</i>	1 x 3 ml	Y.SPR.CS1.MV-3	273,00
<i>Low Value</i>	1 x 3 ml	Y.SPR.CS1.LV-3	273,00

Calibrators - Prediluted Calibrator Sets - Controls**Soluble Transferrin Receptor (sTfR)**

<i>High Value</i>	1 x 1 ml	Y.SPR.STFR.HV	116,00
<i>Low Value</i>	1 x 1 ml	Y.SPR.STFR.LV	116,00